

## Quantification of Corticosteroids and Androgens in Serum, Utilizing Waters MassTrak™ Steroid Serum Sets 2 and Sets 3

---

Laura Moran, Dominic Foley, Niall Tobin, Norma Breen, Leanne Davey

Waters Corporation

*Nur zu Forschungszwecken. Nicht als diagnostisches Verfahren geeignet.*

---

### Abstract

A clinical research method for the quantification of seven endocrine steroid hormones in human serum by UPLC-MS/MS.

### Benefits

- Analytical selectivity of the chromatographic clinical research method provides separation of isobaric species
- LC-MS/MS enables high sample-throughput using multi-well plate automation
- Excellent agreement (within  $\pm 6\%$ ) to the EQA Mass spectrometer mean and in-house panel mean for testosterone, androstenedione, 17-OHP, DHEAS, cortisol, 11-deoxycortisol, and 21-deoxycortisol
- Lyophilized calibrators and QCs that reduce sample preparation time, aid in clinical research method harmonization, and assist with metrological traceability in accordance with ISO 15189:2022.

---

## Introduction

Steroid hormones encompass a large class of small molecules that play a central role in metabolic processes, such as the regulation of sexual characteristics, blood pressure, and inflammation. Enzymes that form part of the steroid biosynthetic pathway are pivotal in these metabolic processes, and their dysfunction can be examined through the correct measurement of steroid hormones in a clinical research setting.

Quantification of steroids is more beneficial using LC-MS/MS, as opposed to traditional ligand binding techniques such as immunoassay, as it can provide higher analytical sensitivity and selectivity and allows for simultaneous quantification of multiple analytes. However, many LC-MS methods lack harmonization or standardization. The Waters MassTrak Steroid Serum Sets (IVD) contains a range of steroid hormones in lyophilized serum that are metrologically traceable to the highest level of metrological traceability available, aiding laboratories in their compliance to ISO 15189, and provide confidence in the accuracy of results.

Waters MassTrak Steroid Serum Cal Set 2 is intended for the quantitative determination of androgens and progestogens in human serum to aid with monitoring of physiological markers. Whilst the MassTrak Steroid Serum Cal Set 3 is intended to be used for the quantitative determination of androgens and glucocorticoids in human serum to aid with monitoring of physiological markers.

Here we describe a clinical research method utilizing Waters MassTrak Steroid Serum Sets 2 and 3, Cals and QCs, and Waters Oasis™ PRiME HLB  $\mu$ Elution plate technology for the extraction of testosterone, androstenedione, 17-hydroxyprogesterone (17-OHP), dehydroepiandrosterone sulfate (DHEAS), Cortisol, 11-deoxycortisol, and 21-deoxycortisol from serum samples, which has been automated using the Hamilton™ Microlab STAR Liquid Handler. Chromatographic separation was performed on a ACQUITY UPLC™ I-Class Plus (FL-I) System, using a ACQUITY UPLC HSS T3 Vanguard™ Pre-Column, and ACQUITY UPLC HSS T3 Column, accompanied by a Xevo™ TQ-S micro Mass Spectrometer (Figure 1).



---

*Figure 1. Waters ACQUITY UPLC I-Class Plus system and Xevo TQ-S micro.*

---

## Experimental

### Sample Preparation

For this study Waters MassTrak Steroid Serum Cal Set 2 (186010563IVD), MassTrak Steroid Serum QC Set 2 (186010564IVD), MassTrak Steroid Serum Cal Set 3 (186010565IVD), and MassTrak Steroid Serum QC Set 3 (186010566IVD) Calibrators and Quality Controls, alongside MassTrak Steroid Internal Standard Mix (186010567IVD) were prepared as per instructions.

MassTrak Steroid Serum Cal Set 2 and Set 3, QC Set 2 and Set 3 contain the following analytes in a range of concentrations.

	Compound	Calibrator range (ng/mL)	QC range (ng/mL)
Set 2	Testosterone	0.01-20	0.03-9
	Androstenedione	0.05-20	0.15-9
	17-OHP	0.1-100	0.3-80
	DHEAS	50-8000	150-5000
Set 3	Androstenedione	0.05-100	0.15-50
	17-OHP	0.3-300	0.5-150
	Cortisol	3-500	9-400
	11-deoxycortisol	0.1-100	0.3-70
	21-deoxycortisol	0.1-100	0.3-70

Table 1. MassTrak Steroid Serum Cal Set 2 and Set 3, QC Set 2, and Set 3 concentration range for each analyte.

(To convert SI units to nmol/L multiply by 3.470 for testosterone (ng/mL to nmol/L), 3.494 androstenedione (ng/mL to nmol/L), 3.028 for 17-OHP (ng/mL to nmol/L), 2.716 for DHEAS (ng/mL to nmol/L), 2.761 for Cortisol (ng/mL to nmol/L), and 2.889 for 11-deoxycortisol and 21-deoxycortisol (ng/mL to nmol/L)).

## Sample Extraction

Prior to extraction it is suggested to centrifuge all samples for 5 mins at 3000 x g. Extraction was performed using the Hamilton Microlab Star Liquid Handler. To 100 µl of sample; 25 µl of MassTrak Steroid Internal Standard Mix was added to each well of sample. (2 ng/mL of testosterone <sup>13</sup>C<sub>3</sub>, 4 ng/mL of androstenedione <sup>13</sup>C<sub>3</sub>, 10 ng/mL of 17OHP <sup>13</sup>C<sub>3</sub>, 3000 ng/mL of DHEAS <sup>2</sup>H<sub>6</sub>, 100 ng/mL of cortisol <sup>13</sup>C<sub>3</sub>, 4 ng/mL of 11-deoxycortisol <sup>13</sup>C<sub>3</sub>, and 10 ng/mL of 21-deoxycortisol <sup>2</sup>H<sub>4</sub>). 200 µl of LC-MS Grade Methanol and 550 µl of LC-MS grade Water is added to each well. The samples are mixed after each reagent addition. Samples then centrifuged for five minutes at 4000 x g.

An aliquot of each of the pre-treated samples (600 µl) was loaded into individual wells of the Oasis PRiME HLB µElution Plate (p/n: 186008052 <<https://www.waters.com/nextgen/global/shop/sample-preparation-->

[filtration/186008052-oasis-prime-hlb-96-well--elution-plate-3-mg-sorbent-per-well-1-p.html](#) ) and slowly pulled through at low vacuum (100 mbar). Consecutive washes with 150 µl of 0.1% (v/v) ammonia in 35% (v/v) methanol<sub>(aq)</sub> and 150µL 0.1% (v/v) formic acid in 35% (v/v) methanol<sub>(aq)</sub> were performed to reduce potential ionic interference. Analytes were eluted into a collection plate using 30 µL of 85/15 (v/v) acetonitrile/methanol, followed by addition of 70 µL water.

## LC Conditions

LC system:	ACQUITY UPLC I Class Plus (FL-I) System
Column(s):	ACQUITY UPLC HSS T3 Column (2.1 x 50 mm, 1.8 µm) (p/n: 186003538)
Pre column:	ACQUITY UPLC HSS T3 Van Guard Pre-Column (p/n: 186003976)
Column temperature:	50 °C
Sample temperature:	10 °C
loopsize:	50 µL
Needle:	20 µL
Injection volume:	20 µL
Injection Mode:	PLNO
Flow rate:	0.6 mL/min
Mobile phase A:	Water with 2 mM ammonium acetate + 0.1% formic acid

Mobile phase B:	Methanol with 2 mM ammonium acetate + 0.1% formic acid
Strong needle wash:	100% Methanol
Weak needle wash:	40% Methanol <sub>(aq)</sub>
Run time:	4.7 min
Gradient:	See Table 1

## MS Conditions

MS system:	Xevo TQ-S micro
Resolution:	MS1 (0.75FWHM), MS2 (0.50FWHM)
Acquisition mode:	Multiple Reaction Monitoring (MRM)
Capillary voltage:	1.0 kV
Polarity:	ESI +/-
Source temperature:	150 °C
Desolvation temperature:	600 °C
Desolvation gas flow:	1000 (L/Hr)
Cone gas flow:	50 (L/Hr)
MS inter-scan delay:	0.01 s

Inter-channel delay: 0.02 s

Polarity/Mode switch interscan: 0.015 s

## Data Management

Chromatography/MS software: MassLynx v4.1 Software with TargetLynx

Time (min)	Flow (mL/min)	%A	%B	Curve
Initial	0.600	55	45	Initial
1.0	0.600	55	45	6
3.5	0.600	35	65	6
3.51	0.600	2	98	11
4.0	0.600	55	45	11

---

*Table 2. Gradient table for the separation of the steroid hormones. Operating back pressure at the initial conditions was approximately 9000–10000psi.*

Compound	Parent ion (m/z)	Product ion (m/z)	Dwell time (s)	Cone (eV)	Collision (V)	ESI mode
Androstenedione (Quan)	287.2	97.0	0.043	45	20	+
Androstenedione (Qual)	287.2	109.0	0.043	45	20	+
Androstenedione <sup>13</sup> C <sub>3</sub>	290.2	100.0	0.043	45	20	+
Testosterone (Quan)	289.2	97.0	0.043	45	20	+
Testosterone (Qual)	289.2	109.0	0.043	45	20	+
Testosterone <sup>13</sup> C <sub>3</sub>	292.2	100.0	0.043	45	20	+
17-OHP(Quan)	331.2	97.0	0.043	55	24	+
17-OHP (Qual)	331.2	109.0	0.043	55	24	+
17-OHP <sup>13</sup> C <sub>3</sub>	334.2	100.0	0.043	55	24	+
DHEAS (Quan)	367.2	97.0	0.03	45	30	-
DHEAS (Qual)	367.2	80.0	0.03	45	75	-
DHEAS <sup>2</sup> H <sub>6</sub>	373.2	98.0	0.03	45	30	-
Cortisol (Quan)	363.2	121.0	0.03	45	24	+
Cortisol (Qual)	363.2	97.0	0.03	45	24	+
Cortisol <sup>13</sup> C <sub>3</sub>	366.2	124.0	0.03	45	24	+
11-Deoxycortisol (Quan)	347.2	97.0	0.03	45	24	+
11-Deoxycortisol (Qual)	347.2	121.0	0.03	45	18	+
11-Deoxycortisol <sup>13</sup> C <sub>3</sub>	350.2	100.0	0.03	45	24	+
21-Deoxycortisol (Quan)	347.2	175.0	0.03	45	30	+
21-Deoxycortisol (Qual)	347.2	121.0	0.03	45	18	+
21-Deoxycortisol <sup>2</sup> H <sub>4</sub> *	351.2	121.0	0.03	45	18	+
21-Deoxycortisol <sup>2</sup> H <sub>4</sub>	351.2	177.0	0.03	45	18	+

\* Alternative product ion.

Table 3. MRM parameters for testosterone, androstenedione, 17-OHP, DHEAS, cortisol, 11- deoxycortisol, and 21-deoxycortisol, and their stable isotope labelled internal standards. The scan window for the analytes were 1.40–2.75 mins for DHEAS, cortisol, 11-deoxycortisol, and 21-deoxycortisol (+/- switching), and 2.76–3.80 mins for testosterone, androstenedione and 17-OHP. Mobile phase was directed to waste at all other times. Dwell times were set to automatic for all analytes, bar DHEAS, which was set to 0.03 s, with 15 points across the peak.

## Results and Discussion

The chromatographic selectivity of the column is demonstrated through the baseline resolution of isobaric



steroid species; 11-deoxycortisol and 21-deoxycortisol (please see Analysis of Corticosteroids and Androgens in Serum for Clinical Research 720005999 <<https://www.waters.com/nextgen/global/library/application-notes/2017/analysis-of-corticosteroids-and-androgens-in-serum.html>> (2017), which demonstrated the separation of 17-OHP and 21-OHP and testosterone and epitestosterone). No significant interferences were observed at the retention time of testosterone, androstenedione, 17-OHP, DHEAS, cortisol, 11-deoxycortisol, and 21-deoxycortisol, when each of these compounds were individually examined. No significant system carryover was observed from high concentration samples into subsequent blank injections. Analytical sensitivity using signal:noise (S/N) of the low calibrator of each set (C1) was >10:1 at each of calibrator 1 concentrations across several analytical runs.

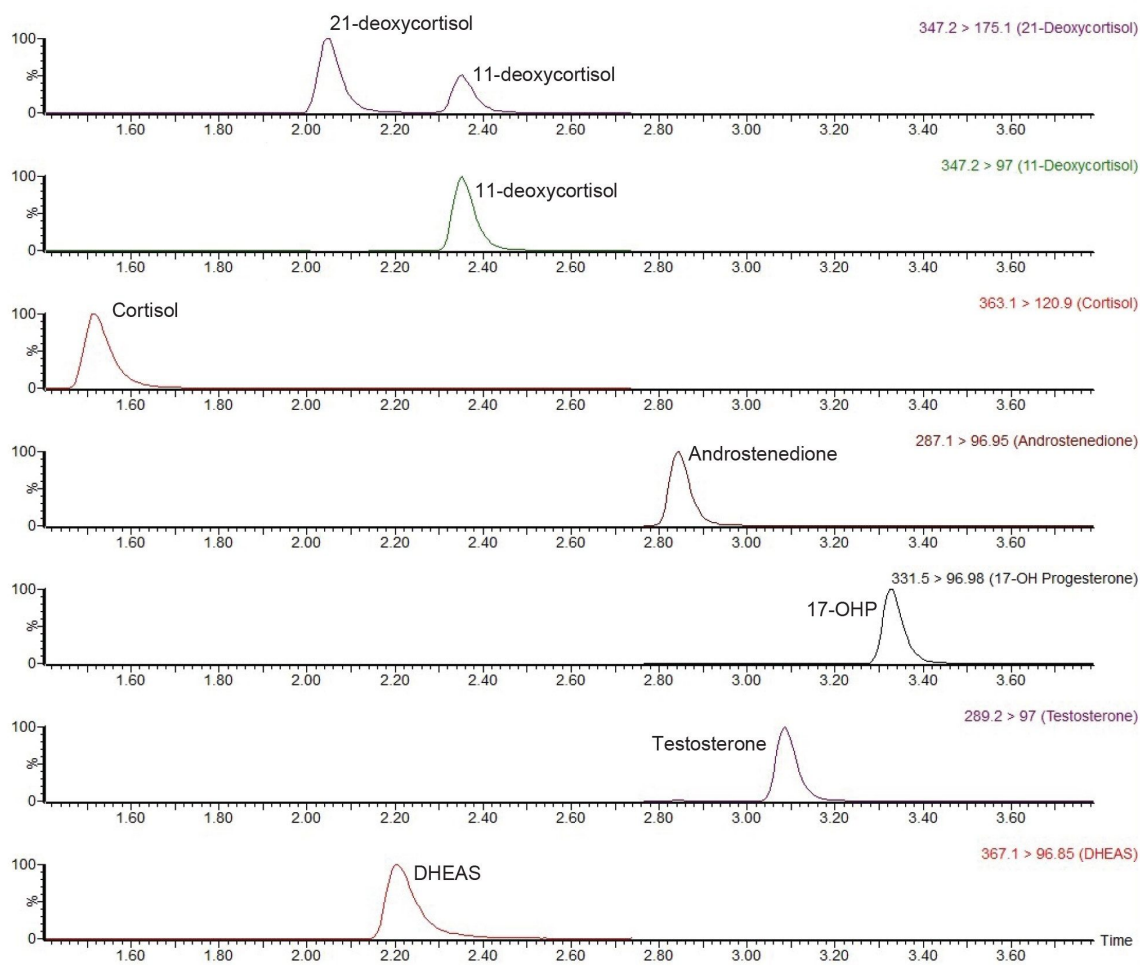


Figure 2. Chromatographic selectivity on the ACQUITY UPLC HSS T3 Column for the selection of steroid hormones.

The clinical research method allows for precise quantification of all analytes at low concentrations. Total precision was determined by extracting and quantifying two replicates per QC level over five days. Repeatability was assessed by analysing four replicates at each QC level in a single analytical run. All results for all analytes were <10%CV, with the majority of results <5%CV.

Set	Compound	Total precision (%CV)				Repeatability (%CV)			
		QC 1	QC 2	QC 3	QC 4	QC 1	QC 2	QC 3	QC 4
Set 2	Testosterone	6.3	2.8	2.6	2.1	3.1	1.8	1.3	0.4
	Androstenedione	2.5	2.3	3.2	3.9	1.5	1.8	1.00	0.8
	17-OHP	2.1	6.9	3.1	5.1	2.2	1.1	1.3	1.0
	DHEAS	3.3	2.7	2.7	3.3	4.8	4.4	2.5	2.0
Set 3	Androstenedione	1.6	1.9	1.7	1.2	0.8	0.8	0.4	1.2
	17-OHP	3.2	1.9	3.4	1.6	1.1	1.5	1.1	0.8
	Cortisol	1.6	1.1	2.2	1.3	0.3	0.5	1.7	0.9
	11-Deoxycortisol	2.2	2.2	2.1	2.1	1.7	1.2	1.4	1.1
	21-Deoxycortisol	9.9	9.0	3.8	3.8	5.7	2.2	3.1	1.7

*Table 4. Total precision and repeatability for the analysis of MassTrak Steroid Serum Cals Set 2 and 3, measuring MassTrak Steroid Serum Set 2 and 3 QC material.*

The clinical research method was shown to be linear for all analytes over the calibration ranges specified in Table 1 when different ratio of low and high concentration pools of the analytes were combined and analysed. Furthermore, calibration lines created using Set 2 and Set 3 were analysed over a five-day period and were linear with a co-efficient of determination of ( $r^2$ ) >0.999 for all analytes.

Set	Compound	Linear coefficient of determination ( $r^2$ )				
		Day 1	Day 2	Day 3	Day 4	Day 5
Set 2	Testosterone	1.0000	0.9998	0.9995	0.9997	0.9999
	Androstenedione	0.9999	0.9999	0.9999	0.9997	0.9980
	17-OHP	1.0000	0.9997	0.9993	0.9994	0.9995
	DHEAS	0.9979	0.9996	0.9978	0.9985	0.9993
Set 3	Androstenedione	0.9998	0.9999	0.9996	0.9999	0.9999
	17-OHP	0.9991	0.9997	0.9988	0.9990	0.9994
	Cortisol	0.9993	0.9999	0.9992	0.9998	0.9998
	11-Deoxycortisol	0.9986	0.9993	0.9997	0.9992	0.9999
	21-Deoxycortisol	0.9999	0.9999	0.9993	0.9996	0.9998

*Table 5. Linear co-efficient of determination for each analyte, in each set, over a five day period.*

Accuracy was assessed for testosterone, androstenedione, 17-OHP, DHEAS, and cortisol through the analysis of EQA material. The data obtained over a four-day period, was compared to the mass spectrometry method mean

for each EQA sample, and the mean % difference from target was tabulated (Table 6). All analytes were assessed at the low, medium, and high end of the calibration line for each MassTrak Steroid Serum Set, which yielded excellent results across the range ( $\pm 10\%$ ). Due to the unavailability of EQA material for 11-deoxycortisol and 21-deoxycortisol, in house panels were used to assess the accuracy of these compounds and the low and medium range. Deming regression and Linear regression was performed (Table 7). No Statistically significant bias was observed for each compound, with a mean method bias of  $\pm 1.3\%$  for Set 2 and  $\pm 1.0\%$  for Set 3.

Compound		Low	Med	High	N=	Mean % diff from target	
Set 2	Testosterone	106%	93%	93%	52	96%	EQA material
	Androstenedione	98%	95%	98%	56	95%	
	17-OHP	93%	107%	110%	56	102%	
	DHEAS	103%	94%	107%	54	101%	
Androstenedione	94%	97%	101%	56	98%		
Set 3	17-OHP	97%	107%	110%	48	102%	In house panels
	Cortisol	107%	104%	101%	42	104%	
	11-Deoxycortisol	98%	106%	n/a	54	102%	
	21-Deoxycortisol	101%	99%	n/a	51	100%	

*Table 6. Accuracy summary table, EQA Material - % Difference of EQA Mean Target for LCMS to Waters measured concentration. Due to the unavailability of EQA material for 11-deoxycortisol and 21-deoxycortisol, in house panels were used to assess the accuracy of these compounds and the low and medium range.*

	Compound	Samples	Deming equation	Mean bias	Linear fit (r)
Set 2	Testosterone	54	$y=0.061 + 0.922x$	-3.93%	1.000
	Androstenedione	58	$y=0.064 + 0.984x$	-3.52%	0.999
	17-OHP	56	$y=-0.298 + 1.109x$	1.50%	0.999
	DHEAS	54	$y=-116.9 + 1.080x$	0.63%	0.999
Set 3	Androstenedione	56	$y=-0.113 + 1.019x$	-2.38%	0.999
	17-OHP	48	$y=-0.210 + 1.102x$	2.13%	1.000
	Cortisol	42	$y=4.028 + 0.995x$	3.49%	0.999
	11-Deoxycortisol	54	$y=-0.027 + 1.063x$	1.73%	1.000
	21-Deoxycortisol	51	$y=-0.003 + 0.994x$	0.05%	0.999

*Table 7. Deming regression comparing Waters LC-MS/MS method to the EQA scheme MS method for testosterone, androstenedione, 17-OHP, DHEAS, and Cortisol analysis. 11-Deoxycortisol and 21-Deoxycortisol comparison to in house panels and medium range.*

## Conclusion

Through this proof of performance evaluation, it has been demonstrated the MassTrak Steroid Serum Calibrator and Quality Control Sets 2 and 3 (IVD) can provide precise and accurate quantification of steroid hormones in serum. An analytically sensitive and selective clinical research method has been developed for the analysis of testosterone, androstenedione, 17-OHP, DHEAS, cortisol, 11-deoxycortisol, and 21-deoxycortisol in serum using Waters Xevo TQ-S micro (FL).

The Xevo TQ-S micro Mass Spectrometer enables this clinical research method to provide sufficient analytical sensitivity to analyse low levels of testosterone, androstenedione, 17-OHP, DHEAS, cortisol, 11-deoxycortisol, and 21-deoxycortisol by using only 100 µL of sample volume.

The assay's accuracy ( $\pm 6\%$ ) and precision ( $\pm 10\%$ ) have been confirmed through comparison to EQA LC-MS/MS means, In House Panels, and QC material for testosterone, androstenedione, 17-OHP, DHEAS, cortisol, 11-deoxycortisol, and 21-deoxycortisol. The addition of automation or liquid handlers, in particular this study utilized the Hamilton Microlab STAR improves laboratory workflow and helps remove operator errors.

## Disclaimer

*This clinical research method is an example of an application using the instrumentation, software, and consumables described in this document. This clinical research method has not been cleared by any regulatory entity for diagnostic purposes. The end user is responsible for completion of the method development and validation. MassTrak Endocrine Steroid Calibrator and Quality Control Sets are not available for sale in all countries. For information on availability, please contact your local sales representative.*

---

## References

Foley D, Calton L. Analysis of Corticosteroids and Androgens in Serum for Clinical Research. Waters Application Note [720005999](#). May 2017.

---

## Featured Products

[ACQUITY UPLC I-Class PLUS System <https://www.waters.com/134613317>](https://www.waters.com/134613317)

[Xevo TQ-S micro Triple Quadrupole Mass Spectrometry <https://www.waters.com/134798856>](https://www.waters.com/134798856)

[MassLynx Mass Spectrometry Software <https://www.waters.com/513662>](https://www.waters.com/513662)

[TargetLynx <https://www.waters.com/513791>](https://www.waters.com/513791)

720008138, December 2023



© 2024 Waters Corporation. All Rights Reserved.

[Nutzungsbedingungen](#) [Datenschutz](#) [Marken](#) [Karriere](#) [Cookies](#) [Cookie-Einstellungen](#)

---